

AD _____

Award Number: DAMD17-99-1-9227

TITLE: Prediction of Malignancy in Breast Tumors Using Diffusion
Weighted Magnetic Resonance Imaging

PRINCIPAL INVESTIGATOR: Paula Gareau, Ph.D.
Brian K. Rutt, Ph.D.

CONTRACTING ORGANIZATION: The John P. Robarts Research Institute
London, Ontario, Canada N6A 5K8

REPORT DATE: July 2000

TYPE OF REPORT: Annual Summary

PREPARED FOR: U.S. Army Medical Research and Materiel Command
Fort Detrick, Maryland 21702-5012

DISTRIBUTION STATEMENT: Approved for Public Release;
Distribution Unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

DTIC QUALITY INSPECTED 3
20010108 170

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 074-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE July 2000	3. REPORT TYPE AND DATES COVERED Annual Summary (1 Jul 99 - 30 Jun 00)	
4. TITLE AND SUBTITLE Prediction of Malignancy in Breast Tumors Using Diffusion Weighted Magnetic Resonance Imaging			5. FUNDING NUMBERS DAMD17-99-1-9227	
6. AUTHOR(S) Paula Gareau, Ph.D. Brian K. Rutt, Ph.D.				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) The John P. Robarts Research Institute London, Ontario, Canada N6A 5K8 E-MAIL: pgareau@irus.rrri.on.ca			8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) U.S. Army Medical Research and Materiel Command Fort Detrick, Maryland 21702-5012			10. SPONSORING / MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION / AVAILABILITY STATEMENT Approved for public release; distribution unlimited				12b. DISTRIBUTION CODE
13. ABSTRACT (Maximum 200 Words) The purpose of this research is to develop a non-invasive predictor of malignancy in breast tumors using novel magnetic resonance imaging (MRI) techniques. The hypothesis is that the spatial distribution of microvasculature around a breast lesion is specific for malignancy and can be reliably measured by a completely non-invasive MRI method. This hypothesis is being tested by: 1) The design and construction of ultra-high gradient coils for MRI. 2) The implementation of advanced MRI pulse sequences for mapping of microvascular parameters 3) The correlation of MRI-derived vascular parameters (diffusion and perfusion) with histological parameters (tumor grade and microvessel density) in an animal model of human breast cancer.				
14. SUBJECT TERMS Breast Cancer, magnetic resonance imaging, angiogenesis, microvessel density, high strength gradient coils, diagnosis			15. NUMBER OF PAGES 12	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT Unlimited	

NSN 7540-01-280-5500

Standard Form 298 (Rev. 2-89)
Prescribed by ANSI Std. Z39-18
298-102

FOREWORD

Opinions, interpretations, conclusions and recommendations are those of the author and are not necessarily endorsed by the U.S. Army.

___ Where copyrighted material is quoted, permission has been obtained to use such material.

___ Where material from documents designated for limited distribution is quoted, permission has been obtained to use the material.

___ Citations of commercial organizations and trade names in this report do not constitute an official Department of Army endorsement or approval of the products or services of these organizations.

N/A In conducting research using animals, the investigator(s) adhered to the "Guide for the Care and Use of Laboratory Animals," prepared by the Committee on Care and use of Laboratory Animals of the Institute of Laboratory Resources, national Research Council (NIH Publication No. 86-23, Revised 1985).

X For the protection of human subjects, the investigator(s) adhered to policies of applicable Federal Law 45 CFR 46.

___ In conducting research utilizing recombinant DNA technology, the investigator(s) adhered to current guidelines promulgated by the National Institutes of Health.

___ In the conduct of research utilizing recombinant DNA, the investigator(s) adhered to the NIH Guidelines for Research Involving Recombinant DNA Molecules.

___ In the conduct of research involving hazardous organisms, the investigator(s) adhered to the CDC-NIH Guide for Biosafety in Microbiological and Biomedical Laboratories.

Pala Gane July 25, 00
PI - Signature Date

Table of Contents

Cover.....	1
SF 298.....	2
Foreword.....	3
Table of Contents.....	4
Introduction.....	5
Body.....	6
Key Research Accomplishments.....	9
Reportable Outcomes.....	10
Conclusions.....	10
Appendices.....	11

Introduction

X-ray mammography is currently the clinically accepted modality for breast cancer screening. Mammography, however, is particularly unreliable and recent trials have shown that 70-80% of mammographically indeterminate lesions that progress to surgical biopsy are benign. The development of accurate, non-invasive imaging tests with low false negative rates would allow reduction of the two step process of surgical biopsy followed by surgical lesion removal to a single step, as well as providing a tool for guiding treatment decisions. It may be possible to achieve this through the development of non-invasive imaging techniques that measure vascular parameters of tumors (for example, blood flow, blood volume, and permeability or microvessel density). Tumor progression is known to depend on the ability to stimulate the growth of new blood vessels that supply nutrients and oxygen to the expanding tumor. This process is known as angiogenesis. It has been hypothesized that the characteristic new vessel growth associated with tumor angiogenesis should allow differentiation between malignant and benign breast lesions. The purpose of this research is to develop a non-invasive predictor of malignancy through the design and preliminary validation of a new form of magnetic resonance imaging (MRI) called the IntraVoxel Incoherent Motion (IVIM) method that utilizes high main magnetic field strength and ultra-strong magnetic field gradients. This is compared with vascular parameters derived from dynamic contrast enhanced MRI.

BODY

Hardware Development

A high strength gradient coil has been designed. The prototype coil was built with an inner diameter of 5cm, which is ideal for mice. A second gradient coil has now been built that is more suitable for rats. This coil has an inner diameter of 24cm, which can accommodate a rat plus the equipment used to monitor the animal. The maximum gradient strength achievable with this coil is 300mT/m, which is almost ten times greater than typical clinical systems and is sufficient for the high-resolution imaging experiments proposed in this grant. This coil is currently being tested at two field strengths: 1.5 and 4.0 Tesla (T). A specialized radiofrequency surface coil was designed and constructed to allow the acquisition of high quality MR data with very high signal to noise.

Implementation of Mammary Tumor Model in Rats

A mammary tumor model has been implemented in female Sprague-Dawley rats using N-ethyl-N-nitrosourea (ENU). ENU is known to be a potent carcinogen that induces well vascularized mammary tumors in rats. This tumor model was chosen because a range of benign and malignant tumors develops depending on the dose of ENU administered and because the tumor morphology and angiogenic behavior closely mimics breast tumors in humans. Mammary tumors developed in 28/30 rats administered a high dose of ENU (180 mg/kg) and in 6/30 rats administered a low dose of ENU (45 mg/kg).

Pulse Sequence Development

Intravoxel Incoherent Motion (IVIM)

The IVIM pulse sequence has been designed based on a standard diffusion-weighted imaging sequence. The sequence consists of a spin echo, echo planar imaging sequence with the addition of strong magnetic field gradients that cause the contrast in the images to be weighted based on the diffusion of water in the microvascular and extra-vascular compartments. We have incorporated a simple phase correction method that allows post-acquisition correction of the images for small scale motion of the object being imaged. Validation of the IVIM sequence has been performed using

phantoms that are spherical containers filled with water and acetone. The results obtained (Appendix I) agree well with those found in the literature.

High signal to noise ratios (SNR) are required in the IVIM images in order to observe the microvascular component of the measured signal. The average SNR in the IVIM images, obtained using the custom-built RF coil, is approximately 400, which we predict is sufficient for this measurement.

Preliminary results (Appendix II) show a fast decay component. The magnitude of the diffusion coefficient for this component is in on the order of that expected for the microvascular blood flow. To verify that the IVIM component is related to microvascular blood flow some animals were imaged before and after sacrifice. This fast decay component disappears after cessation of blood flow. These results suggest that the IVIM method is capable of measuring the tumor microvasculature.

Dynamic Contrast Enhanced MRI (DCE-MRI)

For DCE-MRI we extended a previously developed magnetization prepared 3D SPGR imaging sequence. Rats were imaged before and during bolus contrast agent injection (Gadolinium-DTPA). Axial slices containing both the tumor and the aorta are obtained to allow for determination of the tissue and blood enhancement curves. The tumor blood flow, blood volume and permeability-surface area product were obtained from kinetic analysis of the dynamic tumor enhancement responses.

The accuracy of the DCE-MRI technique is being assessed by comparing DCE-MRI results with computed tomography (CT) data. Dynamic enhanced CT was performed on the same tumor within 24 hours after the DCE-MRI scanning. The CT derived vascular parameters (blood flow, blood volume and mean transit time or permeability) are used as a "gold standard" against which to compare the DCE-MRI derived vascular parameters.

Both IVIM and DCE-MRI images have been obtained from each tumor. Further analysis of the acquired images is underway.

Histologic Analysis

Tumors were removed and prepared for histologic analysis. Formalin-fixed tumors were sliced with guidance from the MR images and digital images taken during the dissection performed to obtain histological tissue slices that correspond to the images slices from which MR measurements are made. The tumors have been resected and a histopathologic analysis is to be performed to determine the microvessel density and spatial distribution, tumor type and tumor grade. The quantitative MRI-derived vascular parameters will be correlated with the histopathologic tumor grade and other markers of tumor angiogenic activity.

Key Research Accomplishments

- Design of a mouse-sized gradient coil with gradient strengths that exceed 2000mT/m. (Approximately 50 to 100 times higher than typical clinical MRI systems.)
- Design of a gradient coil with an inner diameter of 24cm, which is large enough to accommodate a rat and animal monitoring equipment. Maximum gradient strengths achieved with this coil will be 300mT/m.
- Implementation of a breast tumour model in rats that produces tumours with a range of malignancies from benign to malignant.
- Implementation of a fast MR pulse sequence that allows acquisition of diffusion weighted images with high signal to noise.
- Implementation of a dynamic contrast enhanced MR sequence to allow in vivo measurements of tumor blood flow, blood volume and permeability.
- Acquisition of *in vivo* dynamic contrast enhanced MR images and diffusion weighted images of mammary tumors
- Acquisition of dynamic contrast enhanced computed tomography (CT) images, analogous to those acquired using MRI, for comparison of vascular parameters.

Reportable Outcomes

Presentations and Publications

1. The preliminary results of the acquisition and analysis of the images acquired from the animal tumor model were presented at the Era of Hope Meeting, Atlanta, June 8-12, 2000.

Conclusions

We have designed a mouse-sized gradient coil and a gradient coil large enough to accommodate rats and animal monitoring equipment. Both coils achieve gradient strengths significantly higher than typical clinical MRI systems. Based on wire density and power dissipation considerations, we have concluded that small coils with high gradient strengths, such as those required for high resolution IVIM imaging, require multilayer configurations. The design for the coils constructed here should be scalable to a breast-sized coil. Such a coil will allow imaging of the human breast at resolutions that, until now, have been unattainable, thus allowing visualization of very small lesions within the breast.

A carcinogen-induced rat mammary tumor model has been reproduced in our lab. This model produces a wide spectrum of tumor types allowing us to compare the MRI-derived diffusion and perfusion measurements in benign and malignant mammary tumors.

A MR pulse sequence protocol has been implemented at 1.5T for quantitative diffusion and perfusion measurements from rat mammary tumors. The MRI-derived vascular parameters are being compared with histologic scores of tumor aggressiveness, microvesel density and permeability. Preliminary results suggest that these techniques developed have the potential to provide noninvasive measurements of the microvasculature in breast tumors. This would allow diagnosis of breast lesions *in vivo* and would also provide a means of following the effects of treatments, particularly treatment with anti-angiogenic pharmaceuticals; however, further testing of our methods is required before definitive conclusions can be drawn.

Appendix I

The IVIM method and the analysis program developed for this grant were tested with two substances – water and acetone - whose diffusion coefficients are well documented. The theoretical and experimentally determined results are shown below for diffusion encoding along six different directions:

Water:

The theoretical value of the diffusion coefficient of water is between 2.12×10^{-3} and $2.63 \times 10^{-3} \text{ mm}^2/\text{s}$ at 21.7°C .

<u>Diffusion Encoding Direction</u>	<u>Diffusion Coefficient (mm^2/s)</u>
xy	$2.03 \pm 0.02 \times 10^{-3}$
-xy	$2.10 \pm 0.09 \times 10^{-3}$
xz	$2.08 \pm 0.10 \times 10^{-3}$
-xz	$1.97 \pm 0.06 \times 10^{-3}$
yz	$2.07 \pm 0.04 \times 10^{-3}$
-yz	$2.07 \pm 0.11 \times 10^{-3}$


Acetone:

The theoretical value of the diffusion coefficient of acetone is between 3.88×10^{-3} and $4.43 \times 10^{-3} \text{ mm}^2/\text{s}$ at 21.7°C .

<u>Diffusion Encoding Direction</u>	<u>Diffusion Coefficient (mm^2/s)</u>
xy	$4.47 \pm 0.04 \times 10^{-3}$
-xy	$4.59 \pm 0.05 \times 10^{-3}$
xz	$4.62 \pm 0.03 \times 10^{-3}$
-xz	$4.30 \pm 0.05 \times 10^{-3}$
yz	$4.47 \pm 0.06 \times 10^{-3}$
-yz	$4.55 \pm 0.06 \times 10^{-3}$

Appendix II

Shown below are the bi-exponential diffusion coefficients before (D_A , D_B) and after (D_X , D_Y) cessation of blood flow (euthanasia) in non-necrotic regions of interest in low and high dose tumours.

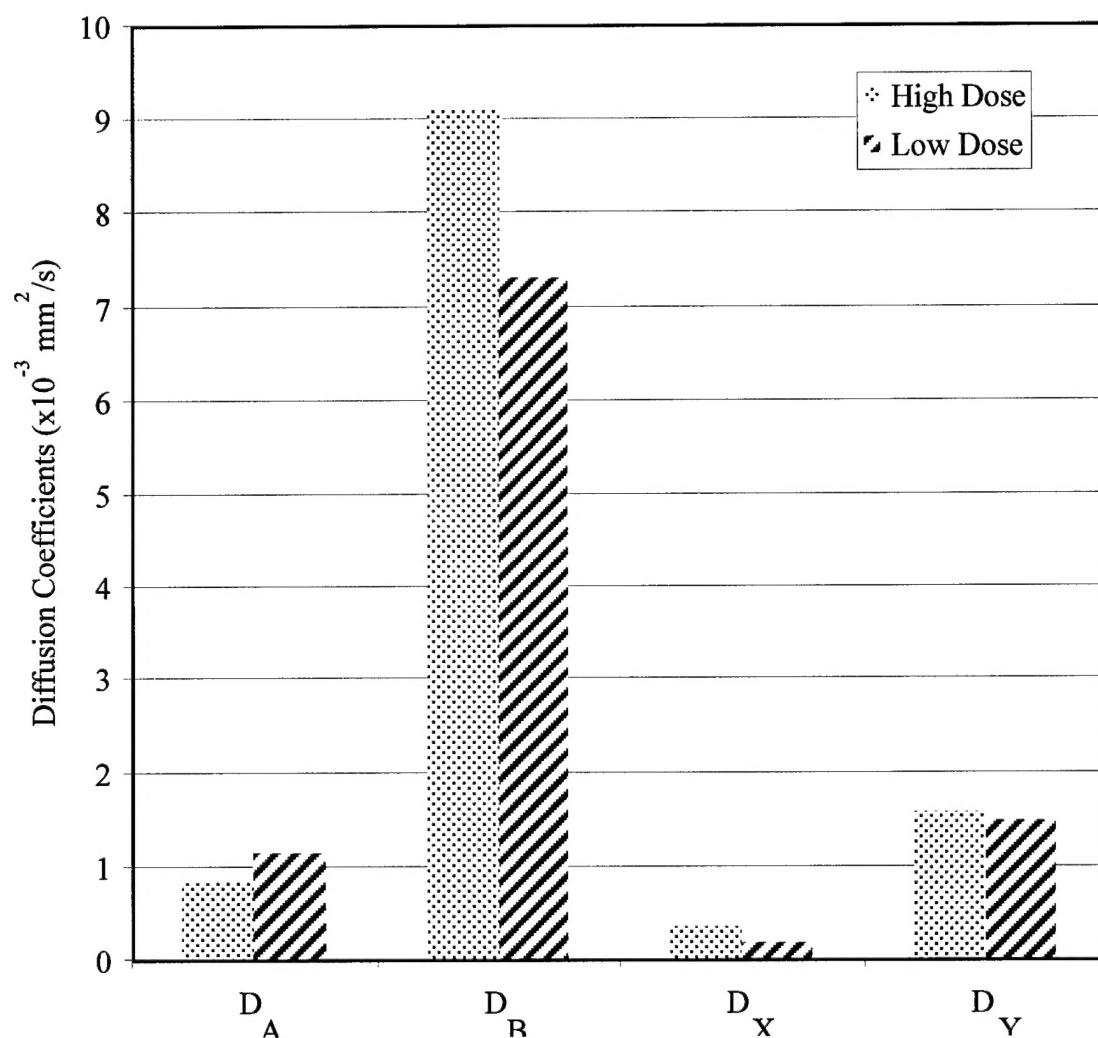

Note that the fast decay component (large diffusion coefficient), D_B , disappears post cessation of blood flow. The presence of a bi-exponential decay post cessation of blood flow may be attributed to different rates of diffusion in the intra- and extracellular spaces. We are currently endeavoring to assign these two diffusion components.